

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWM-0025
Location:	CLIFTON CITY POLICE	
Calibration File No.:	00768	Calib. Date: 03/20/2009
Certification File No.:	00769	Calib. No.: 00016
Linearity File No.:	00770	Cert. Date: 03/20/2009
Solution File No.:	00829	Cert. No.: 00009
Sequential File No.:	00829	Lin. Date: 03/20/2009
		Lin. No.: 00009
		Soln. Date: 05/27/2009
		Soln. No.: 00071
		File Date: 05/27/2009
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0032
Solution Control Lot:	07J048	Expires: 10/03/2009
		Bottle No.: 1067

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:40D		
Control 1 EC	0.100%	16:40D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:40D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:41D		
Control 2 EC	0.099%	16:42D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:42D		
Control 3 EC	0.099%	16:43D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	16:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:44D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BRANCATO

First Name: DAVID

MI: A

Signature: \_\_\_\_\_



Badge No.: 10

Date: 05/27/2009



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
Post Office Box 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

JON S. CORZINE
Governor

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 11/28/07

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 07J048

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1225 to 0.1229 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 3, 2009.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ajit R. Tungare]

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 17th day of December, 2007.

[Handwritten signature of Linda L. DeSantis]
Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009




New Jersey is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF

**State**  
**and**  
**Public**  
**Safety**

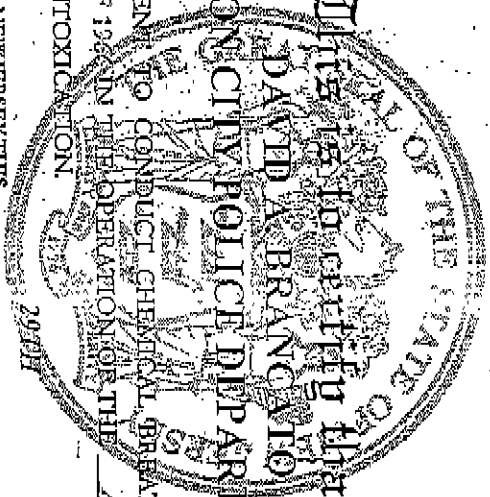

CLIFTON CITY POLICE DEPARTMENT  
DAVID A. BRANCA TO

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 710 MKIII-C,  
A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS

29<sup>TH</sup>

DAY OF

MARCH

TWO THOUSAND AND SIX

*Joseph L. Mend*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*Richard V. Parker*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

DEPARTMENT OF  
**Motor and Public Safety**  
*Up to its quality that*

David Francato  
 Clifton Police Department

QUALIFIED AND COMPETENT TO CONDUCT THIS COURSE IN ACCORDANCE WITH THE REQUIREMENTS OF CHAPTER 17C OF THE LAWS OF 1964 IN THE REGULATION OF THE STATE OF NEW JERSEY AND TO CERTIFY TO THE COMPLETION OF THIS COURSE TO THE DEPARTMENT OF MOTOR AND PUBLIC SAFETY.  
 A NOTED TO DEVELOPER IN THE FOLLOWING MANNER:  
 GIVEN UNDER MY HAND AND SEAL OF THE STATE OF NEW JERSEY ON the 20th DAY OF February

IN WASHINGTON AND HIGHWAY

*[Signature]*  
 SUPERVISOR  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES 3-29-2006

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>2-7-08</u>	<u>Sussex Co. PA</u>	<u>Russo</u>
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 253B (Rev. 07/07)