

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARWM-0025
Location: CLIFTON CITY POLICE
Calibration File No.: 00904 Calib. Date: 09/03/2009 Calib. No.: 00017
Certification File No.: 00905 Cert. Date: 09/03/2009 Cert. No.: 00010
Linearity File No.: 00906 Lin. Date: 09/03/2009 Lin. No.: 00010
Solution File No.: 00974 Soln. Date: 11/05/2009 Soln. No.: 00080
Sequential File No.: 00974 File Date: 11/05/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXA S3-0033
Control Solution %: 0.100% Expires: 01/15/2011
Solution Control Lot: 09A062 Bottle No.: 1177

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 17:49S | | |
| Control 1 EC | 0.103% | 17:50S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.103% | 17:50S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 17:50S | | |
| Control 2 EC | 0.101% | 17:51S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.103% | 17:51S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 17:52S | | |
| Control 3 EC | 0.102% | 17:52S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.102% | 17:52S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 17:53S | | |

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: BRANCATO

First Name: DAVID

MI: A

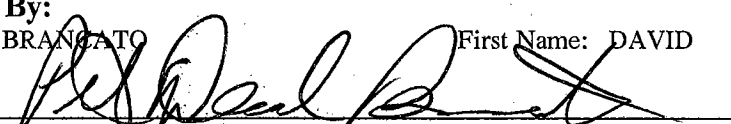Signature: 

Badge No.: 10

Date: 11/05/2009



JON S. CORZINE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
Post Office Box 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATHE ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 2/11/2009

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 09A062

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1195 to 0.1197 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 15, 2011.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police


Sworn to and subscribed before me this 20th day of February, 2009.

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009



DEPARTMENT OF

Ita for **Standard** *Reubolite* **Safes**



This is to certify that
DAVID A. BRANCAPIO
CLIFTON CITY POLICE DEPARTMENT

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO
CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 29TH DAY OF MARCH

TWO THOUSAND AND SIX

Joseph P. ...
SUPERINTENDENT
NEW JERSEY STATE POLICE

Julius V. ...
ATTORNEY GENERAL
STATE OF NEW JERSEY

DEPARTMENT OF
Health and Public Safety
 This is to certify that

David Brancato
 Clifton Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
 THE LAWS OF 1946 IN THE OPERATION OF THE **ALCOHOL 7110 MK III C**
 A METHOD TO DETERMINE INTOXICATION
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, THE 20th DAY OF February

[Signature]
 SHERIFF
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES 3-29-2006

| DATE | Refresher Course PLACE | INSTRUCTOR |
|------------------|------------------------|--------------|
| 1. <u>2-7-08</u> | <u>Sussex Co. PA</u> | <u>Russo</u> |
| 2. _____ | _____ | _____ |
| 3. _____ | _____ | _____ |
| 4. _____ | _____ | _____ |
| 5. _____ | _____ | _____ |
| 6. _____ | _____ | _____ |
| 7. _____ | _____ | _____ |
| 8. _____ | _____ | _____ |
| 9. _____ | _____ | _____ |

S.P. 2938 (Rev. 07/07)