

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARWM-0025
Location:	CLIFTON CITY POLICE	
Calibration File No.:	02001	Calib. Date: 12/19/2014
Certification File No.:	02002	Cert. No.: 00033
Linearity File No.:	02003	Cert. Date: 12/19/2014
Solution File No.:	02032	Lin. No.: 00022
Sequential File No.:	02032	Soln. No.: 00186
		File Date: 04/22/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXA S3-0033
Solution Control Lot:	13G115	Expires: 07/15/2015
		Bottle No.: 0755

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:37D		
Control 1 EC	0.101%	14:38D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	14:38D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:38D		
Control 2 EC	0.101%	14:39D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	14:39D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:40D		
Control 3 EC	0.101%	14:40D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.102%	14:40D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:41D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: TURANO

First Name: PETER

MI: A

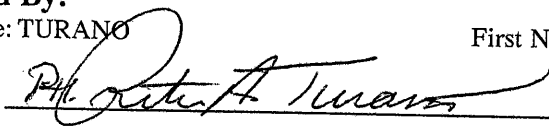
Signature: 

Badge No.: 204

Date: 04/22/2015

DEPARTMENT OF

# Motor Vehicle Safety



This is to certify that  
Peter A. Furano  
Clifton City Police Department

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO  
CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 7110 MKIII-C  
A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS Twelfth DAY OF June

TWO THOUSAND AND Nine

*Joseph P. ...*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*Gene ...*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

DEPARTMENT OF  
**Law and Public Safety**  
 This is to certify that

**Peter A. Turano**  
 Clifton City Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF  
 THE LAWS OF 1966 IN THE OPERATION OF THE **ALCOTEST 7110 MKIII-C**  
 A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THE 12th DAY OF June  
 TWO THOUSAND AND Nine

*[Signature]*  
 SUPERINTENDENT  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 11/21/11	BCPA	R. W.
2. 11/13/13	S.C.C.S.T.A.	R. D.
3.		
4.		
5.		
6.		
7.		
8.		
9.		



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL

DEPARTMENT OF LAW AND PUBLIC SAFETY

DIVISION OF STATE POLICE

POST OFFICE BOX 7068

WEST TRENTON, NJ 08628-0068

(609) 882-2000

CHRIS CHRISTIE  
Governor

KIM GUADAGNO  
Lt. Governor

JOHN J. HOFFMAN  
Acting Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

CERTIFICATION OF ANALYSIS

0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.

ANALYSIS DATE: 7/29/2013

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 13G115

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1213 to 0.1220 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 18, 2015.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouié, Ph.D.  
Research Scientist  
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 7<sup>th</sup> day of August, 2013.

Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable

